

Protocol for Apoptosis Assay by Flow Cytometry Using Annexin V Staining Method

Imayavaramban Lakshmanan and Surinder K Batra*

Biochemistry and Molecular Biology, Nebraska Medical Center, Omaha, USA

*For correspondence: sbatra@unmc.edu

[Abstract] This assay is used to count the number of cells that have undergone apoptosis. Apoptosis will be detected by initially staining the cells with Annexin V and propidium iodide solution followed by flow cytometry analysis. It is based on the principle that normal cells are hydrophobic in nature as they express phosphatidyl serine in the inner membrane (side facing the cytoplasm) and when the cells undergo apoptosis, the inner membrane flips to become the outer membrane, thus exposing phosphatidyl serine. The exposed phosphatidyl serine is detected by Annexin V, and propidium iodide stains the necrotic cells, which have leaky DNA content that help to differentiate the apoptotic and necrotic cells.

Materials and Reagents

1. Annexin V FLUOS staining kit (F. Hoffmann-La Roche, catalog number: 11858777001)
2. The kit contains ready-to-use Annexin-V-FLUOS solution, propidium iodide solution, and incubation buffer
3. Trypsin
4. NaCl
5. KCl
6. Na₂HPO₄
7. KH₂PO₄
8. PBS buffer (pH 7.4) (see Recipes)

Equipment

1. Flow cytometer
2. Centrifuge
3. T25 culture flask

Procedure

1. Seed cells (1 x 10⁶ cells) in a T25 culture flask (in triplicate for experiments) and three

- T25 culture flask for control (unstained, Annexin only, and propidium iodide only).
- After 48 h incubation, collect the supernatant (floating apoptotic cells) and trypsinize the adherent cells (~2 x 10⁶ cells) from each T25 flask (combine respective floating and trypsinized cells resulting in six tubes).
 - Wash the collected cells twice with PBS and centrifuge (670 x g, 5 min, RT).
 - Re-suspend each pellet (~2 x 10⁶ cells) in PBS (400 µl).

For experimental cells (Triplicate) - (400 µl of cells + 100 µl of incubation buffer with 2 µl of Annexin [1 mg/ml] and 2µl of propidium iodide [1 mg/ml]).

For control cells

Control 1: (unstained) - (without any stain (400 µl of cells + 100 µl of incubation buffer)

Control 2: (Annexin V only) - (400 µl of cells + 100 µl of incubation buffer with 2 µl of Annexin (1 mg/ml))

Control 3: (propidium iodide only) - (400 µl of cells + 100 µl of incubation buffer with 2 µl of propidium iodide (1 mg/ml))

- Analyze the cells using a flow cytometry without washing the cells
- Cells that were propidium iodide (PI) negative and Annexin V negative are considered healthy, cells, PI negative and Annexin V positive cells are considered apoptotic, and cells that are positive to both PI and Annexin V considered necrotic (Figure 1).

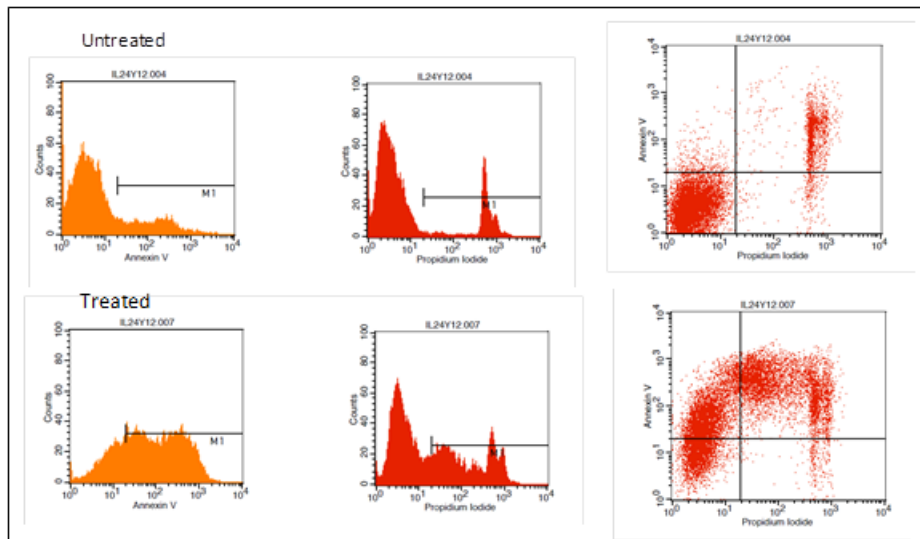


Figure 1.

Recipes

- PBS buffer (pH 7.4)
8 g NaCl

0.2 g KCl

2.3 g Na₂HPO₄

0.22 g KH₂PO₄

In 800 ml of distilled H₂O adjust the pH to 7.4.

Acknowledgments

The authors thank Dr. Palanimuthu Ponnusamy Moorthy and Dr. Dhanya Haridas for critical reading of the apoptosis experimental protocol. We also thank Philip Hexley and Victoria Smith, Flow Cytometry Research Facility at UNMC, for their support.

References

1. Lakshmanan, I., M. P. Ponnusamy, S. Das, S. Chakraborty, D. Haridas, P. Mukhopadhyay, S. M. Lele and S. K. Batra (2012). [MUC16 induced rapid G2/M transition via interactions with JAK2 for increased proliferation and anti-apoptosis in breast cancer cells](#). *Oncogene* 31(7): 805-817.